

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
27 May 2004 (27.05.2004)

PCT

(10) International Publication Number
WO 2004/044573 A1

(51) International Patent Classification⁷: G01N 27/414, (74) Agent: REINHOLD COHN AND PARTNERS; P.O.Box 33/543 4060, 61040 Tel Aviv (IL).

(21) International Application Number:
PCT/IL2003/000941

(22) International Filing Date:
11 November 2003 (11.11.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
152746 11 November 2002 (11.11.2002) IL

(71) Applicant (for all designated States except US): YISSUM RESEARCH DEVELOPMENT COMPANY OF THE HEBREW UNIVERSITY OF JERUSALEM [IL/IL]; Hi Tech Park, Edmond Safra Campus, Givat Ram, 91390 Jerusalem (IL).

(72) Inventors; and

(75) Inventors/Applicants (for US only): YITZCHAIK, Shlomo [IL/IL]; 6/1 Davidson Street, 93708 Jerusalem (IL). SPIRA, Micha [IL/IL]; 7 Malki Street, Yemin Moshe, 94102 Jerusalem (IL). SHAPPIR, Joseph [IL/IL]; 30 Hermon Street, 90805 Mevasseret Zion (IL).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: TRANSISTOR-BASED BIOSENSORS HAVING GATE ELECTRODES COATED WITH RECEPTOR MOLECULES

(57) Abstract: A device and method are presented for detecting analyte molecules in a medium. At least one FET (Field Effect Transistor) is provided being formed by at least one pair of source-drain electrodes and at least one gate electrode. The gate electrode is coated with a layer of receptor molecules that in the presence of said analytes catalyze a reaction that causes release of ions in a medium surrounding said receptor molecules. A monolayer of linker molecules is provided for linking said receptor molecules to said at least one gate such that a distance between the receptor molecules layer and the surface of the coated gate is smaller than 15Å. In the preferred embodiments, the receptor molecules are enzymes (e.g. acetylcholine esterase) or peptides, and the analyte molecules are pesticides, herbicides and chemical pollutants of industrial origin.

BEST AVAILABLE COPY

WO 2004/044573 A1

- 1 -

TRANSISTOR-BASED BIOSENSORS HAVING GATE ELECTRODES COATED WITH RECEPTOR MOLECULES

FIELD OF THE INVENTION

This invention relates to a biosensor for the detection of molecules. More specifically, the present invention relates to a biosensor that incorporates an enzyme.

5 REFERENCES

- Cahn, T.M. and Jackson, S.A., Biosensors, Chapman & Hall, Paris, 1991.
- Coulet, P.R., "From chemical sensors to bioelectronics: a constant search for improved selectivity, sensitivity, and miniaturization", Proceedings of the scientific Computing and Automation (Europe).
- 10 Gopel, W., Heiduschka, P., Introduction to bioelectronics: interfacing biology with electronics, Biosens., Bioelectron., 1994, iii-xiii.
- Gorchkov, D.V., Soldatkin, A.P., Poyard, S., Jaffrezic-Renault, Martelet, N., C., Application of charged polymeric materials as additional permselective membranes for improvement of the performance characteristics of urea-sensitive enzymatic field effect transistors: 1. Determination of urea in model solutions, 15 Mater. Sci. Eng., C 5, 1997, 23-28.
- Jimenez, C., Bartoli, J., de Rooij, N.F., Koudelka-Hep, M., Use of photopolymerizable membranes based on polyacrylamide hydrogels for enzymatic microsensor construction, Anal. Chim. Acta. 351, 1997, 169-176.
- 20 Kharitonov, A.B., Shipway, A.N., Willner, I., An Au-nanoparticle bis-bipyridinium cyclophane-functionalized ion-sensitive field-effect transistor for the sensing of adrenaline, Anal. Chem. 71, 1999, 5441-5443.
- Kharitonov, A.B., Zayats, M., Lichtenstein, A., Katz, E., Willner, I., Enzyme monolayer-functionalized field-effect transistors for biosensor applications,

- 2 -

Sensors and Actuators B., 70, 2000, 222-231.

Powner E.T., Yalcinkaya F., Intelligent Biosensor, Sensor Review, Vol.17, No.2,1997, pp.107-116.

Senillou, A., Jafferezic-Renault, N., Martelet, C., Cosnier, S, A miniaturized
5 urea sensor based on the integration of both ammonium based urea enzyme field effect transistor and a reference field effect transistor in a single chip, Talanta 50, 1999, 219-226.

Sze, S.M., Semiconductors Sensors, Wiley, New York, NY, 1994, pp. 127-8.

Turner, A.P.F., Karube, I. And Wilson, G.S., Biosensors, Fundamentals And
10 Applications, Oxford University Press, Oxford, 1987, p.5.

Wise, D.L., Applied Biosensors, Butterworths, London, 1989, pp. 93-114.

BACKGROUND OF THE INVENTION

The Integration of biologically active molecules with electronic transducers has emerged as an elegant and effective way of creating high fidelity
15 systems for the detection of a wide range of biological activities (Turner, 1987; Gopel, 1994; Cahn, 1991). The aim of such biological sensory systems is the production of an electrical signal which is proportional to the concentration of a certain biochemical agent, and thus reflects the level of biochemical activity of the biocatalyst involved (Powner, 1997). Such systems serve as translators of
20 biological events into electrical signals and can prove to be the link between the much-understood world of silicon-based electronics and the biological world.

The high specificity of biomolecules such as enzymes, antibodies, etc. allows for the creation of reaction-specific biosensory systems that can be used for a wide array of applications (Coulet).

25 A review of sensor technology may be found in Sze (1994). One type of sensor technology prepared in the past concerns the use of ion-sensitive field-effect transistor (ISFET) in which the normal metal-oxide-silicon field-effect transistor (MOSFET) gate electrode is replaced by an ion-sensitive membrane with the ability to detect ion concentrations in solution (Wise, 1989), as

- 3 -

schematically shown in Fig. 1.

Enzyme-based sensory systems such as the traditional enzyme-based field-effect transistors (ENFET) and enzyme-electrodes have also been described in the past (Jimenez, 1997; Senillou, 1999; Gorchkov, 1997; Kharitonov, 1999, 5 2000).

SUMMARY OF THE INVENTION

The inventors have found that a Field Effect Transistor (FET) may be used as a sensor for molecules in solution and air, and may be used specifically to monitor catalytic activity of an enzyme assembled thereon. This is achieved by 10 coating a gate electrode of the FET with a layer of receptor molecules that in the presence of certain analytes can catalyze a reaction that causes release of ions in a medium surrounding said receptor molecules, and providing a monolayer of linker molecules for linking said receptor molecules to said gate such that the distance between the receptor molecules layer and the surface is smaller than 15 15Å. Preferably, this distance is of about a few angstroms.

Thus, according to one aspect of the present invention, there is provided a device for the detection of analyte molecules, the device comprising at least one pair of source-drain electrodes and at least one gate electrode to thereby define at least one Field Effect Transistor (FET), wherein said at least one gate electrode is 20 coated with a layer of receptor molecules that in the presence of said analytes catalyze a reaction that causes release of ions in a medium surrounding said receptor molecules, and a monolayer of linker molecules is provided for linking said receptor molecules to said at least one gate such that a distance between the receptor molecules layer and the surface of the coated gate is smaller than 15Å.

25 The receptor molecules are preferably enzymes or peptides, and more preferably enzyme molecules. One specifically preferred enzyme is acetylcholine esterase (AChE).

- 4 -

Thus, according to another broad aspect of the invention, there is provided a device for the detection of analyte molecules, the device comprising at least one pair of source-drain electrodes and at least one gate electrode to thereby define at least one Field Effect Transistor (FET), wherein said at least one gate electrode is coated with a layer of receptor molecules including acetylcholine esterase (AChE) that in the presence of analytes including acetylcholine catalyzes a reaction that causes release of ions in a medium surrounding said receptor molecules, and a monolayer of linker molecules is provided for linking said receptor molecules to said at least one gate such that a distance between the receptor molecules layer and the surface of the coated gate is smaller than 15Å, said linker molecules being selected from conjugated or unconjugated aliphatic, aromatic or heteroaromatic molecules, having at least one functional group capable of covalently binding to said surface and at least one functional group capable of covalently binding to said receptor molecules.

The analyte molecules to be detected by the device of the present invention may be those selected from chemical agents used in agriculture, in environmental applications, industry and chemical warfare. The chemical agents are pesticides, herbicides, nerve agents and synthetic or natural toxins emitted from industrial plants.

The Field Effect Transistor is an Ion Sensitive Field Effect Transistor. The gate electrode is an ion sensitive oxide gate. The ion-sensitive oxide is preferably Aluminum Oxide (Al_2O_3), Silicon Nitride (Si_3N_4), Indium Tin Oxide ($\text{In}_2\text{O}_3\text{-Sn}_2\text{O}_3$), Silicon Oxide (SiO_2) or Tantalum Oxide (Ta_2O_5).

The device may include an array of differently coated gate electrodes, which may be associated with the same source-drain pair, or with different source-drain pairs.

According to another aspect of the present invention, there is provided a method of detecting analyte molecules in a medium, the method comprising:

- 5 -

- (a) providing at least one Field Effect Transistor (FET) formed by a source-drain electrode pair and at least one gate electrode that is coated with a layer of receptor molecules that in the presence of certain analytes catalyze a reaction that causes release of ions in a medium surrounding said receptor molecules, and a monolayer of linker molecules for linking said receptor molecules to said at least one gate such that a distance between the receptor molecules layer and the surface of the coated gate is smaller than 15Å.
- (b) accommodating said at least one FET such that said at least one gate is exposed to a medium suspected of containing analyte molecules capable of reacting with the receptor molecules, thereby affecting a release of ions in said medium, and
- (c) monitoring a change in an electric current between the source and drain electrodes caused by the release of ions, said change being indicative of the presence of said analyte in the medium, thereby enabling measuring the analyte concentration in the medium.

The medium may be one of the following: water, sea water, buffer, and ionic solution.

ABBREVIATIONS

- ISFET- Ion-sensitive field effect transistor; CyC- Cyanuric chloride; I_{ds} - drain-source current; TSA- topotactic self-assembly; ACh- Acetylcholine; AChE- Acetylcholine esterase; DTNB- 5,5'-dithio-bis (2-nitrobenzoic acid); TNB- thionitrobenzoic acid.

BRIEF DESCRIPTION OF THE DRAWINGS

- The present invention will be more fully understood and appreciated from the following detailed description, taken in conjugation with the examples and drawings, in which:

Fig. 1 shows a standard metal-oxide-silicon field-effect transistor (MOSFET, left) and an Ion-Sensitive Field Effect Transistors (ISFETs, right). In an

- 6 -

ISFET the metal oxide gate electrode is replaced by an ion sensitive membrane by which changes in ionic concentrations in solutions induce a change in ISFET transduction that can be measured by drain-source current (I_{ds}).

Fig. 2 shows the stepwise construction of the layered structure. In step (A),
5 Cyanuric Chloride is reacted with the oxide layer of the ISFET gate surface to form covalent linkage. In step (B), the covalently bound cyanuric chloride layer forms a covalent linkage (arbitrary Lysine residue of enzyme) the enzyme.

Fig. 3 shows the experimental (ellipsometry data taken at 75°) Ψ and Δ as a function of wavelength for a monolayer of CyC on Silicon substrate. Based on the
10 complete fitting between the model and experimental results as shown in this Figure, the thickness of the layer was determined.

Fig. 4 represents the hydrolysis of acetylcholine to choline in the presence of AChE in water. The reaction results in the generation of acetic acid and protonation of the solution.

15 **Fig. 5** shows the Acetylcholine dose response of the assembled AChE-FET structure.

Fig. 6 shows the AChE inhibition by eserine as detected by the AChE-FET structure of the present invention.

Fig. 7 shows the response of the structure of the present invention to
20 application of carbamylcholine in comparison with Ach.

Fig. 8 exhibits the ability of the AChE-FET structure to detect small Ach quantities through Ach iontophoresis.

Fig. 9 shows the UV-Vis absorption spectrum of TSA derived CyC monolayer on quartz substrate.

25 **Fig. 10** shows the absorption spectra of 1.25×10^{-4} M of ACh and 5×10^{-5} M DTNB solution before (having a peak at 325 nm) and after (having a peak at 410 nm) a 15-minute exposure to AChE containing substrate.

Fig. 11 shows the absorption spectra of 1.25×10^{-4} M ACh and 5×10^{-5} M DTNB solution exposed to AChE containing substrate, recorded in-situ at 20-
30 second interval.

- 7 -

Fig. 12 represents the optical density at 410nm versus time following the insertion of a glass substrate containing immobilized AChE into 2.5×10^{-4} M ACh and 5×10^{-5} M DTNB solution.

Fig. 13 shows Reaction velocity verses ACh concentration for the surface-bound AChE.

Fig. 14 represents a graphical determination of K_m and V_{max} for the surface bound AChE.

Fig. 15A-B show substrate dependency of ISFET responsiveness: (A) ACh-Iodine dosage response, and (B) basic characterization shows a substantial change in the ISFET transduction and amplification (dI/dV).

Figs. 16A-B show the effects of AChE inhibition by Eserine on I_{ds} . (A) Eserine was injected to the buffer solution at $t = 75$ and at $t = 400$ sec. Acetylcholine was not washed from solution. A major decrease in I_{ds} of the enzyme modified ISFET was observed and a return to a lower I_{ds} level occurred within 50 sec of application. (B) Eserine had very little effect on non enzyme modified ISFET. Acetylcholine was injected at $t = 230$ and at $t = 400$ sec and showed I_{ds} increase. Eserine was injected at $t = 610$ sec and showed similar effects, suggesting response of non-enzyme modified ISFET is merely an artifact.

Fig. 17 depicts the ISFET long term fidelity. AChI-induced response has been measured after 1 month at 4°C and no apparent deterioration of enzyme layer was observed. (AChI was applied at $t = 50$ and at $t = 160$ sec.).

DETAILED DESCRIPTION OF THE INVENTION

In the following, the invention will be illustrated in reference to some non-limiting specific embodiments.

Fig. 1 illustrates MOSFET and ISFET structures suitable to be used in a device of the present invention for the detection of molecules. Generally, the device of the present invention is a FET, in which a gate electrode is formed with a layer of enzyme molecules capable of catalyzing a reaction that causes release of ions in

- 8 -

a media surrounding said enzyme, and a monolayer of linker molecules linking said enzyme to said gate such that the distance between the enzyme and the surface is smaller than 15Å.

The media surrounding said enzyme may be air, water, sea water, buffer
5 solution, ionic solution and others.

Fig. 2 exemplifies how a conventional FET (ISFET in the present not limiting example) can be modified to obtain the device of the present invention. As shown, the gate surface layer Al_2O_3 is coated with cyanuric chloride (constituting linking molecules) which covalently binds to the oxide atoms and is then reacted
10 with the AChE (constituting receptor molecules) which binds covalently to the linking molecules through one of the reactive functional groups of the enzyme.

The enzyme may be a natural or synthetic, preferably selected from the following: proteases, lipases, RNases, DNases, peptidases, glucose oxidase, urease, chymotrypsin, butyrylcholine esterase and acetylcholine esterase. More preferably,
15 the enzyme is acetylcholine esterase, herein designated AChE.

The ion sensitive oxide coat (gate surface layer) may be Aluminum Oxide (Al_2O_3), Silicon Nitride (Si_3N_4), Indium Oxide-Titanium Oxide ($\text{In}_2\text{O}_3\text{-TiO}_3$), Silicon Oxide (SiO_2) or Tantalum Oxide (Ta_2O_5).

The linker molecules are positioned between and covalently bound to both
20 the oxide-coat of the gate and the receptor molecules layer (e.g., enzyme). The linker molecules are preferably selected from conjugated or unconjugated aliphatic, aromatic or heteroaromatic molecules, having at least one functional group capable of covalently binding to said surface and at least one functional group capable of covalently binding to said receptor molecules (enzyme). The term "heteroaromatic"
25 refers to aromatic compounds containing one to three heteroatoms selected from N, O and/or S. The heteroaromatic molecules are for example, and without limiting to pyridyl, pyrrolyl, furyl, thienyl, imidazolyl, oxazolyl, quinoliny, thiazolyl, pyrazolyl, 1,3,4-triazinyl, 1,2,3-triazinyl, benzofuryl, isobenzofuryl, indolyl, imidazo[1,2-a]pyridyl, benzimidazolyl, benzthiazolyl, benzoxazolyl, and
30 quinazolinyl.

- 9 -

These linker molecules bind the receptor molecules to the surface such that the distance between the receptor and the surface is less than 15Å, preferably less than 10Å and most preferably less than 5Å. The thickness of the layer may be determined by various methods, one of which being as shown in Fig. 3.

5 Such linker molecules are for example and without being limiting to short chain aliphatic molecules or mono- or polycyclic aromatic or heteroaromatic molecules capable of forming a single compact layer on the surface of the gate. Surface binding functional groups may for example be halides, activated halides, trichlorosilanes, trialkoxysilanes or other similar groups capable of binding
10 covalently to the surface of the device.

Receptor molecules' bonding groups, capable of binding to functional groups of the receptor molecules may for example be, without being limiting to, halides (i.e. I, Br, Cl), aldehydes, carboxylic acids, active esters, acyl halides and ketones.

15 The linker molecules are preferably heteroaryl compounds substituted by at least one surface-binding functional group and additionally by at least one enzyme-binding functional group; both functional binding groups are preferably labile groups.

The FET device according to the invention serves as an amplifier that
20 translates the presence and concentration of the analyte molecules (i.e. molecules being tested for) on its surface into a change in the electrical current between the source and drain, I_{ds} .

The device of the present invention utilizing an ISFET operates in the following manner. When the receptor molecules (enzyme) on the top of the ion-sensitive layer of the ISFET is brought in contact with an inhibitor of the receptor
25 molecules, free hydrogen ions are formed (as a reaction result), the surface potential on ion sensitive layer changes, thus influencing the current I_{ds} between the drain and source, which makes this current I_{ds} directly related to the pH. The current changes can be detectable either by using a reference electrode screened

- 10 -

from the environment (e.g., from the analyte molecules), or by utilizing a threshold-based programming means.

Enzyme-catalyzed reactions may alter the pH at the ISFET gate surface, either positively, by the uptake of protons, or negatively, by the generation of
5 protons. Such pH changes result in an electrical activity at the gate surface of the transistor and induce current changes between the drain and source electrodes, when the gate-source potential is kept constant.

In one embodiment of the present invention, the ISFET device comprises a an aluminum oxide (Al_2O_3) gate which is covered with a layer of cyanuric chloride
10 molecules and a layer of the AChE enzyme being covalently bound to the cyanuric chloride layer.

AChE catalyses the hydrolysis of acetylcholine, resulting in the generation of acetic acid and choline as shown in **Fig. 4**. The generation of acetic acid and the acidification of the buffer solution induce a pH change that is recorded by the
15 ISFET.

Fig. 5 illustrates experimental results of the Acetylcholine dose response of the AChE-FET structure of the present invention. In this experiment, the ISFET has undergone covalent bonding with acetylcholine-esterase using the aforementioned cyanuryl chloride techniques. As shown in the figure, the
20 response of the AChE-ISFET to various doses of acetylcholine (graph I). Acetylcholine was manually applied into a solution of 5ml Phosphate Saline Buffer (PBS) in which the ISFET resided. The response is sigmoid-shaped and clearly correlates with normal enzyme kinetics: the lowest concentration detectable thus far is 10^{-8} M, while saturation of response has been reached at
25 approximately 0.05M. Bare ISFETs, that haven't undergone the AChE bonding process showed little if any response to the application of Acetylcholine (graph II), excluding response to high concentrations ($>0.1\text{M}$), which might be a consequence of changes in ionic strength of the entire solution or spontaneous Ach hydrolysis. (fast response time of about 2sec shown in the insert, dose is
30 0.001ACh).

- 11 -

Fig. 6 illustrates experimental results of Acetylcholine esterase Inhibition by Eserine detected by AChE-ISFET. Increasing doses of acetylcholine were applied in varying concentrations of Eserine (a reversible and competitive AChE inhibitor) in solution. Total inhibition is observed in 100 μ M Eserine. The same
5 ACh dose response analysis in lower concentrations of Eserine shows a distinct recovery of ISFET voltage in response to Ach. Response in the presence of 0.01 μ M Eserine resembles response without inhibitor (not shown). Thus, the structure of the present invention is able to detect levels of AChE Eserine inhibition in the range of 0.01 μ M to 100 μ M.

10 Fig. 7 illustrates the results of exposing the structure of the present invention to Carbamylcholine which produces no response in comparison to application of ACh. Carbamylcholine ($C_6H_{15}ClN_2O_2$) acts as a cholinergic agonist that is resistant to the action of cholinesterases. When applied to the solution in which the AChE-ISFET resides, no response is evoked, in contrast to the full-scale
15 response evoked by the application of acetylcholine. This is indicative of that the sensor of the present invention is capable of specifically detecting ACh in solution. Both carbamylcholine and acetylcholine have been dissolved in phosphate buffered saline (PBS).

Fig. 8 illustrates the results of ACh Iontophoresis onto AChE-ISFETs.
20 Iontophoresis experiments were conducted using the ISFETs of the present invention that have undergone the AChE bonding process. ACh was inserted into a glass micropipette, which was then brought within distance of approximately 5 μ m from the gate surface of the ISFET. Negative current pulses (200msecs) were then applied onto the micropipette with increasing amplitudes, thus releasing doses of
25 ACh in increasing size. A constant (DC) positive current was applied to prevent leakage of Ach from pipette, and prevent depolarization. In contrast to negative pulses that resulted in the release of Ach and the ISFET's response, negative pulses did not result in a similar or reverted response (not shown). This shows that the ISFET responds specifically to Ach, and furthermore, demonstrates its ability to
30 detect small and local Ach release. Iontophoresis experiments using bare ISFETs

- 12 -

resulted in little or no response. Using standard Ohm's -Law calculations, ISFET's peak sensitivity has been determined to be approximately 20,000 Ach molecules. This is indicative of the capability of the structure of the present invention for sensing quanta release beyond a certain threshold.

5 Examples of the various applications of the device of the present invention, without being limited to are: (1) detection of pesticides and herbicides in agriculture, (2) detection of residual natural and/or synthetic toxins, pesticides and/or herbicides in water, (3) detection of residual natural and/or synthetic toxins, pesticides and/or herbicides in food and food products, (4) detection of synthetic
10 toxins emitted from industrial plants in the air and water, (5) detection of chemical warfare agents, and (6) detection of AChE inhibitors, or agonists.

By utilizing an array of differently coated gates, either associated with the same source-drain pair, or relating to different FETs, such that each gate is composed of a different receptor molecules layer, different analyte molecules can
15 be detected. The invention further relates to a method of detecting analyte molecules and measuring their concentration in air or in solution, e.g., water, sea water, buffer or ionic solution. The device or an array thereof is exposed as disclosed hereinbefore to a medium suspected of containing analyte molecules capable of reacting with the receptor molecules. The change in the current
20 measured at a constant or variable electric potential applied between the source and drain is monitored, and the presence of said analyte is determined.

The determination may be qualitative, although the extent of change may serve as a quantitative measure for the level of said analyte in the medium.

The invention will be further illustrated by the following non-limiting
25 examples.

EXAMPLES

General

Acetylcholine esterase (C1682, taken from electric eel), acetylcholine-
30 iodine, acetylcholine-chloride, cyanuric chloride and eserine (physostigmine),

- 13 -

were purchased from Sigma and were used as supplied.

Measurements were taken in a standard phosphate buffer (PBS), and physiological solutions at room temperature.

Example 1: Solid-State Assembly of Cyanuric Chloride (CyC) on Glass,

5 **Quartz and Silicon**

In order to study the structure-activity relationship and enzyme activity, chemisorption of cyanuric chloride (CyC) was carried out on glass, quartz and silicon wafers. The chlorides of the CyC are very labile and can undergo fast nucleophilic substitution reaction with the substrate (hydroxy containing
10 surfaces) via topotactic self-assembly (TSA).

In this method the substrate (1 inch², active area of 1 mm²) is positioned on a spin-coater holder and wetted with a 0.1 M solution of CyC dissolved in dichloromethane. Spinning at 4000 rpm for 30 seconds resulted in a physisorbed layer of about 60-80 nm in thickness. The covalent bonding onto the surface is
15 achieved by introducing the coated substrate into a vacuum oven (3 mTorr) at 74°C for 10 minutes. These conditions are the optimized balance between the surface reaction kinetics and the sublimation rate of CyC. As the TSA assembly is a self-cleaning solvent-less surface reaction, a mono-molecular layer is obtained.

20 Contact angle measurement of water on the substrate after monolayer assembly gave a wetting angle of -77° as compared with the low wetting angle of -15° obtained with the clean unassembled substrate. Such a high contact angle is characteristic of a hydrophobic interface lacking the ability to form hydrogen bonds with the water droplet. Additionally, it shows a pinhole free monolayer
25 coverage with no hydrophilic interaction with the under laying substrate.

Variable angle spectroscopy ellipsometry (VASE) of the CyC monolayer showed a thickness of 6.7Å for this layer on top of 18Å thick oxide layer. The derived ellipsometric thickness suggests that the alignment of the coupling molecule is perpendicular to the surface and is composed of a single monolayer.

Fig. 9 shows the UV-Vis absorption spectrum of the CyC monolayer. The λ_{max} at 230nm corresponds to the CyC absorption while the OD suggests a molecular number density in the order of 10^{14} molecules/cm².

5 **Example 2: Surface Anchoring of Acetylcholinesterase (AChE)**

A stock solution of the enzyme is prepared by mixing 10 μ l AChE with 100 μ l PBS buffer at pH=7.4. The condensation reaction with the enzyme is obtained by placing a 10 μ l the enzyme solution on the CyC containing substrate in a covered Pettri dish for 10h at 16°C. The unreacted enzyme is then washed off
10 with PBS buffer at pH=7.4, three times. Substrates containing immobilized enzyme were kept under buffered solution at 16°C prior performing the various characterization tests.

To examine whether the immobilization procedures rendered the enzymatic activity, the following experiments were performed.

15 **(a) Enzyme Activity by Ellman's Method.**

In this test, the enzyme activity is measured by following the increase of yellow color produced from the reaction of thiocholine with the DTNB ion (Sawada, O., Ishida, T., Kihachiro, H., J. Biochem., 129, 2001, 899-907) .

The reaction of acetylthiocholine-iodide with DTNB (5,5'-dithio-bis (2-
20 nitrobenzoic acid) marker was conducted by immersing the solid substrate containing the immobilized AChE, obtained above, in an optical cell compatible with the spectrophotometer. The rate of color production was measure at 410nm. All of the investigated solutions were freshly prepared: ACh in phosphate buffer of pH=8.0 and the DTNB dissolved in PBS buffer of pH=6.5.

25 The enzyme activity was probed by two methods: Ex-situ and In-situ experiments. In the Ex-situ experiments the solution of the marker containing ACh is measured before and after the exposure to the immobilized AChE substrate. The optical cell contains a solution composed of 2ml of $2.5 \cdot 10^{-3}$ M ACh and 2ml of $1 \cdot 10^{-4}$ M DTNB. The optical spectra were recorded before and

– 15 –

after 15 min of the immobilized enzyme solution insertion to this optical cell. In the In-situ experiments, the substrate is immersed in the optical cell containing various concentrations of the DTNB/ACh solution. The hydrolysis product was followed in two ways: (a) by recording the spectra in fixed time interval and (b) by the time course mode at 410nm.

Fig. 10 shows the appearance of the 410nm peak of TNB, the reaction product of DTNB and thiocholine and the absorption of DTNB at 325nm before the exposure to the enzyme containing substrate.

Fig. 11 demonstrates the progress of the reaction by the decrease in DTNB absorption and the increase in TNB absorption. The existence of an isosbestic point at 360nm confirms the direct transformation between the two species.

The determination of AChE activity was conducted by probing in real time the absorption of the TNB product at 410 nm. **Fig. 12** exemplified the bio-catalytic activity of the surface bound AChE on the hydrolysis of ACh (in a given concentration) to yield thiocholine. The hydrolysis kinetics is characterized by an initial fast hydrolysis (“the linear regime”) that levels-off with the total consumption of the marker by the hydrolysis product. The slope of the “linear” part ($\Delta A/\Delta t$) can yield the reaction velocity in M/sec.: where $\Delta A = \epsilon \times \Delta C \times l$ ($\epsilon = 14150 \text{ M}^{-1} \cdot \text{cm}^{-1}$ at 412nm and $l = 1 \text{ cm}$).

(b) Reaction Velocity

Repeating the experiment with different ACh concentrations was conducted in order to give the reaction velocity dependence on the substrate concentration as shown in **Fig. 13**. In these experiments the DTNB concentration was kept constant ($5 \times 10^{-5} \text{ M}$).

This bio-catalytic activity of the surface-bound AChE fits the Michaelis-Menten model for enzyme kinetics. At constant enzyme concentration the reaction velocity reaches a saturation value, which is defined as V_{max} . This is consistent with the fact that the number of active sites in the sample is constant and can't react faster with the increase in substrate concentration.

- 16 -

Michaelis-Menten model's defines K_m as the substrate's concentration that yields half the velocity of V_{max} . A Lineweaver-Burk plot, shown in **Fig. 14**, was used for the graphical extraction of these kinetic parameters (see Figure G). The linear regression of the data in the Lineweaver-Burk plot yield: $K_m = 3.1 \times 10^{-4} M$ and $V_{max} = 1 \times 10^{-7} M \text{ sec}^{-1}$, it is worth noting that these values are highly dependent on the experimental conditions such as pH, temperature and ionic-strength.

These tests indicate that the covalent assembly of AChE to a glass substrate via CyC coupling layer preserved the bio-catalytic activity of the enzyme towards the hydrolysis of ACh. This may be concluded from the V_{max} and K_m values that are comparable to those of the free enzyme in solution.

Example 3: ISFET Device Fabrication

ISFETs were first rinsed with isopropanol and dried under Argon. A solution of 0.1M cyanuric chloride (in dichloromethane) was prepared and then applied to the Al_2O_3 gate surface of the ISFET. ISFETs were then dried with Argon and heated at 70°C for 15 minutes, then rinsed again with dichloromethane and dried under Argon. Acetylcholine esterase, 0.1M, was applied onto the modified gate surface and left for 1hr at room temperature, and then rinsed with PBS.

Example 4: The Measurements

The resulting hybrid system of Example 3, was immersed in a PBS solution as a background electrolyte for the measurements. A standard Ag/AgCl electrode was used as the reference electrode. The current between source and drain electrodes (I_{ds}) was measured, while potential between drain and source electrodes (V_{ds}), and between the gate and source electrodes (V_{gs}) were kept constant at 0.1V and 0.45V, respectively, recording the electrical activity occurring at the gate surface.

The substrate dependence of the drain-source current recorded by the

- 17 -

modified ISFET correlates with normal enzyme activity analysis and is shown in Fig. 15A. The modified ISFET showed responsiveness at concentrations of as low as at 10^{-8} M. The response plateau is observed at concentrations in the range of 1mM (not shown). Basic characterization of ISFET transduction was carried out before and after ACh-Iodine or ACh-chloride application (Fig. 15B). A substantial increase in ISFET transduction was observed in correlation with dosage response.

The application of eserine - a reversible acetylcholine esterase inhibitor (Used for medical purposes) - to the solution (without washing ACh) resulted in a major decrease of drain-source current (Fig. 16A). Return of I_{ds} to levels was slightly lower than those before the application of eserine. These results may indicate that the acidification of the solution by the hydrolysis of acetylcholine is halted by eserine only locally, e.g. the esterase activity is halted until sufficient amounts of substrate is diffused to the gate area. Eserine is charged at physiological pH, a fact that could have explained the decrease in I_{ds} . However, the application of eserine onto a non-enzyme-functionalized ISFET has been shown to have opposite effects (Fig. 16B). A minor increase in I_{ds} was recorded which strengthens the suggestion that the effect of eserine is due the inhibition of enzyme activity. Furthermore, the reversible nature of AChE inhibition by eserine correlates with the current increase and may explain this phenomenon.

The long-term fidelity of the enzyme-functionalized ISFETs was also analyzed. ISFETs responsiveness has shown no major decrease in after 30 days in 4°C (Fig. 17). Such high fidelity is non-existent in traditional enzyme based sensors and offers stability and reuse of sensor.

The response time of the sensor is reflected by the amount of time it takes for I_{ds} to reach steady state after the application of the substrate. The average response time of the enzyme modified ISFET was measured under different concentration and was found to be approximately 35 seconds. The response time under low substrate concentrations ($10\mu\text{M}$ - $50\mu\text{M}$) was lower than response time under high concentrations ($100\mu\text{M}$ and above).

CLAIMS:

1. A device for the detection of analyte molecules, the device comprising at least one pair of source-drain electrodes and at least one gate electrode to thereby define at least one Field Effect Transistor (FET), wherein said at least one gate electrode is
5 coated with a layer of receptor molecules that in the presence of said analytes catalyze a reaction that causes release of ions in a medium surrounding said receptor molecules, and a monolayer of linker molecules is provided for linking said receptor molecules to said at least one gate such that a distance between the receptor molecules layer and the surface of the coated gate is smaller than 15Å.
- 10 2. A device according to claim 1, wherein said distance is of a few angstroms.
3. A device according to claim 1 or 2, wherein the Field Effect Transistor is an Ion Sensitive Field Effect Transistor.
4. A device according to any one of preceding claims, wherein the receptor molecules are enzymes or peptides.
- 15 5. A device according to claim 4, wherein the receptor molecules is acetylcholine esterase.
6. A device according to any one of preceding claims, wherein said analyte molecules are selected from chemical agents used in agriculture, in environmental applications, industry and chemical warfare.
- 20 7. A device according to claim 6, wherein said chemical agents are pesticides, herbicides, nerve agents and synthetic or natural toxins emitted from industrial plants.
8. A device according to any one of preceding claims, wherein said gate electrode is an ion sensitive oxide gate.
- 25 9. A device according to claim 8, wherein the ion-sensitive oxide is Aluminum Oxide (Al_2O_3), Silicon Nitride (Si_3N_4), Indium Tin Oxide ($\text{In}_2\text{O}_3\text{-Sn}_2\text{O}_3$), Silicon Oxide (SiO_2) or Tantalum Oxide (Ta_2O_5).
10. A device according to claim 1, wherein said linker molecules are covalently bound to at least one of the surface or the receptor molecules.

- 19 -

11. A device according to claim 8, wherein said linker molecules are selected from conjugated or unconjugated aliphatic, aromatic or heteroaromatic molecules, having at least one functional group capable of covalently binding to said surface and at least one functional group capable of covalently binding to said receptor
5 molecules.
12. A device according to any one of preceding claims, comprising an array of gate electrodes each gate electrode being coated with receptor molecules layer different from that of the other gate electrodes.
13. A device according to claim 12, wherein said array of gate electrodes is
10 associated with the same source-drain pair.
14. A device according to claim 12, wherein each of the gate electrodes is associated with a different source-drain pair.
15. A method of detecting analyte molecules in a medium, the method comprising:
- (a) providing at least one Field Effect Transistor (FET) formed by a source-
15 drain electrode pair and at least one gate electrode that is coated with a layer of receptor molecules that in the presence of certain analytes catalyze a reaction that causes release of ions in a medium surrounding said receptor molecules, and a monolayer of linker molecules for linking said receptor molecules to said at least one gate such that a distance between the receptor
20 molecules layer and the surface of the coated gate is smaller than 15Å.
 - (b) accommodating said at least one FET such that said at least one gate is exposed to a medium suspected of containing analyte molecules capable of reacting with the receptor molecules, thereby affecting a release of ions in said medium, and
 - 25 (c) monitoring a change in an electric current between the source and drain electrodes caused by the release of ions, said change being indicative of the presence of said analyte in the medium, thereby enabling measuring the analyte concentration in the medium.
16. A method according to claim 15, wherein said medium is one of the following:
30 water, sea water, buffer, and ionic solution.

1/14

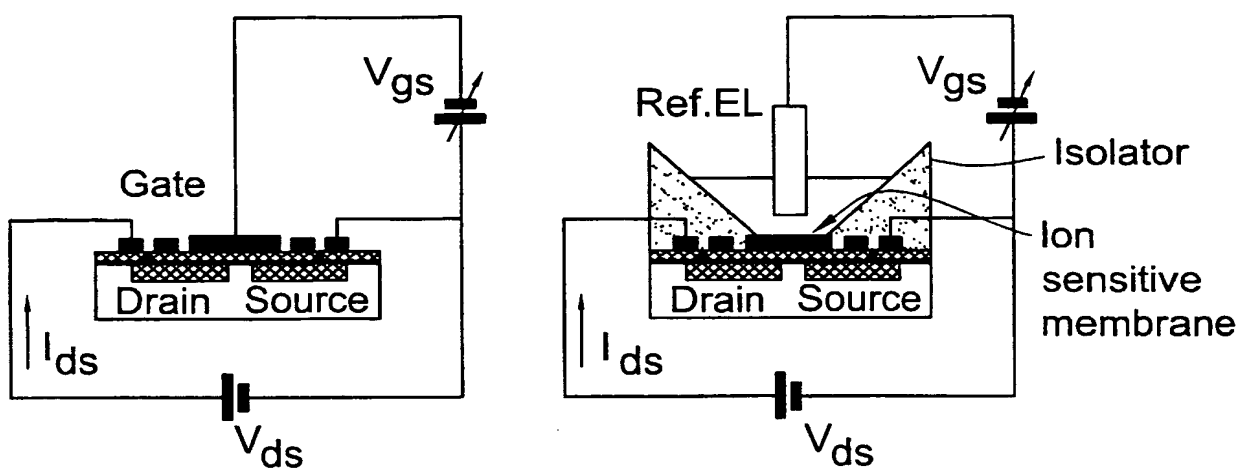


FIG. 1

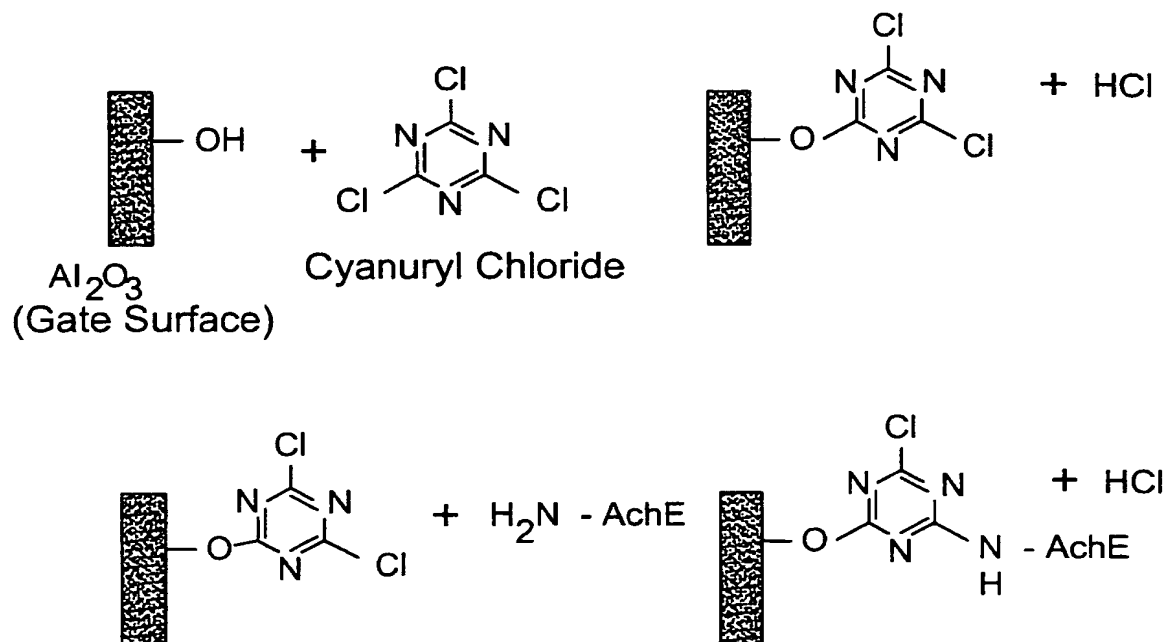


FIG. 2

2/14

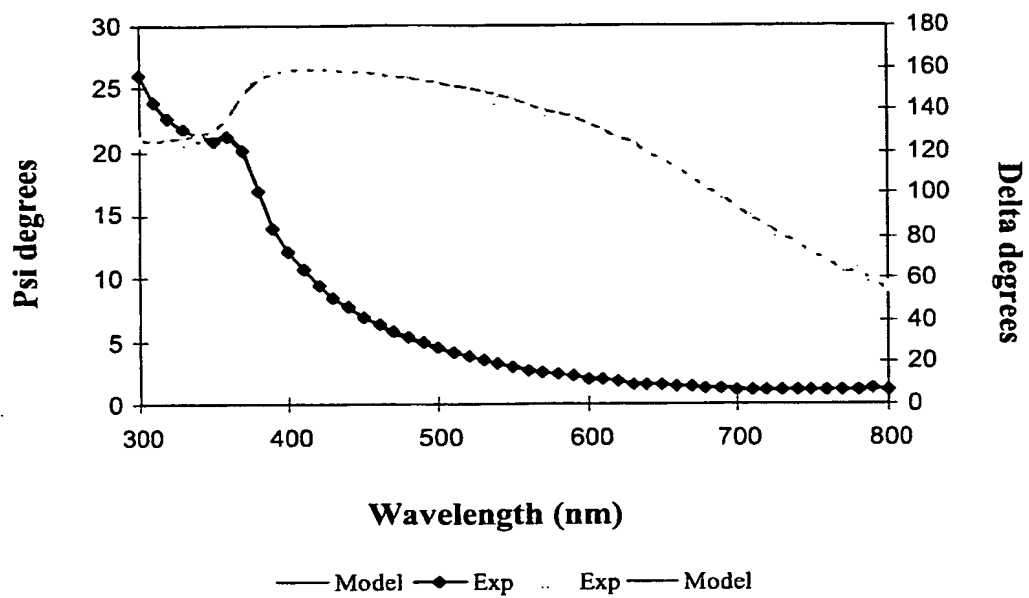


FIG. 3

3/14

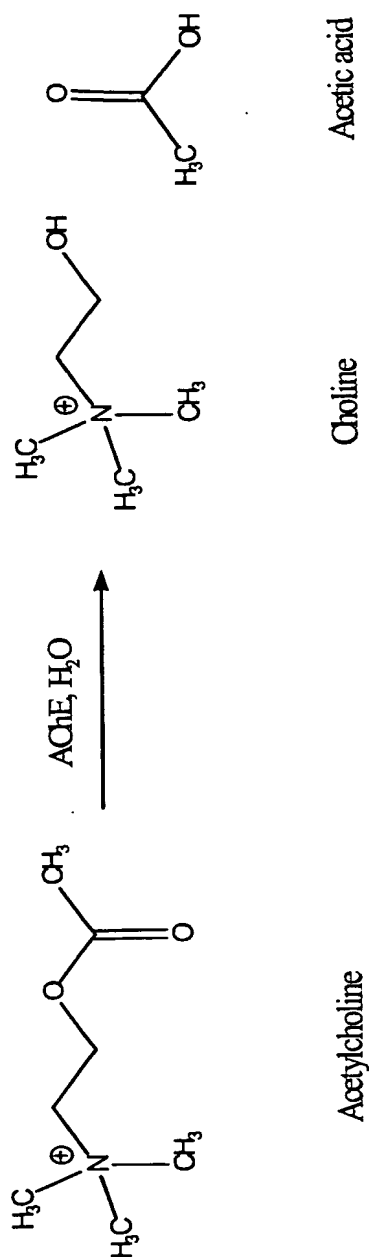


FIG. 4

4/14

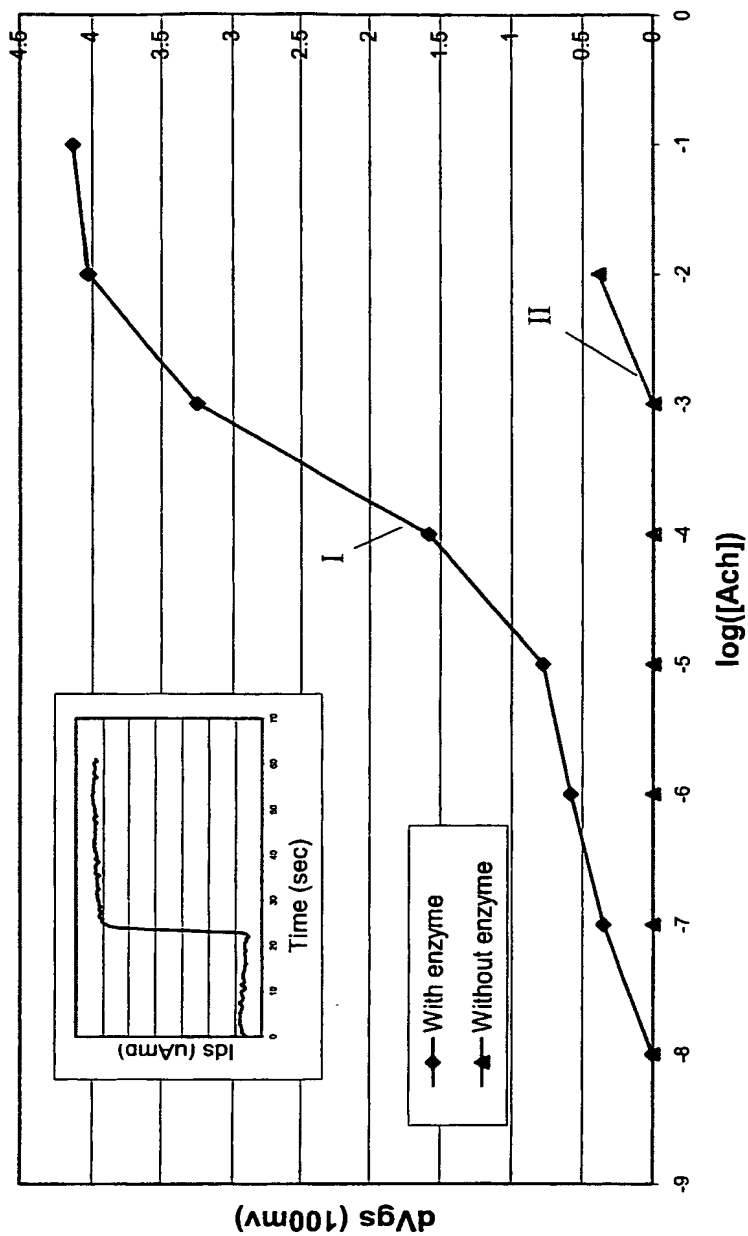


FIG. 5

5/14

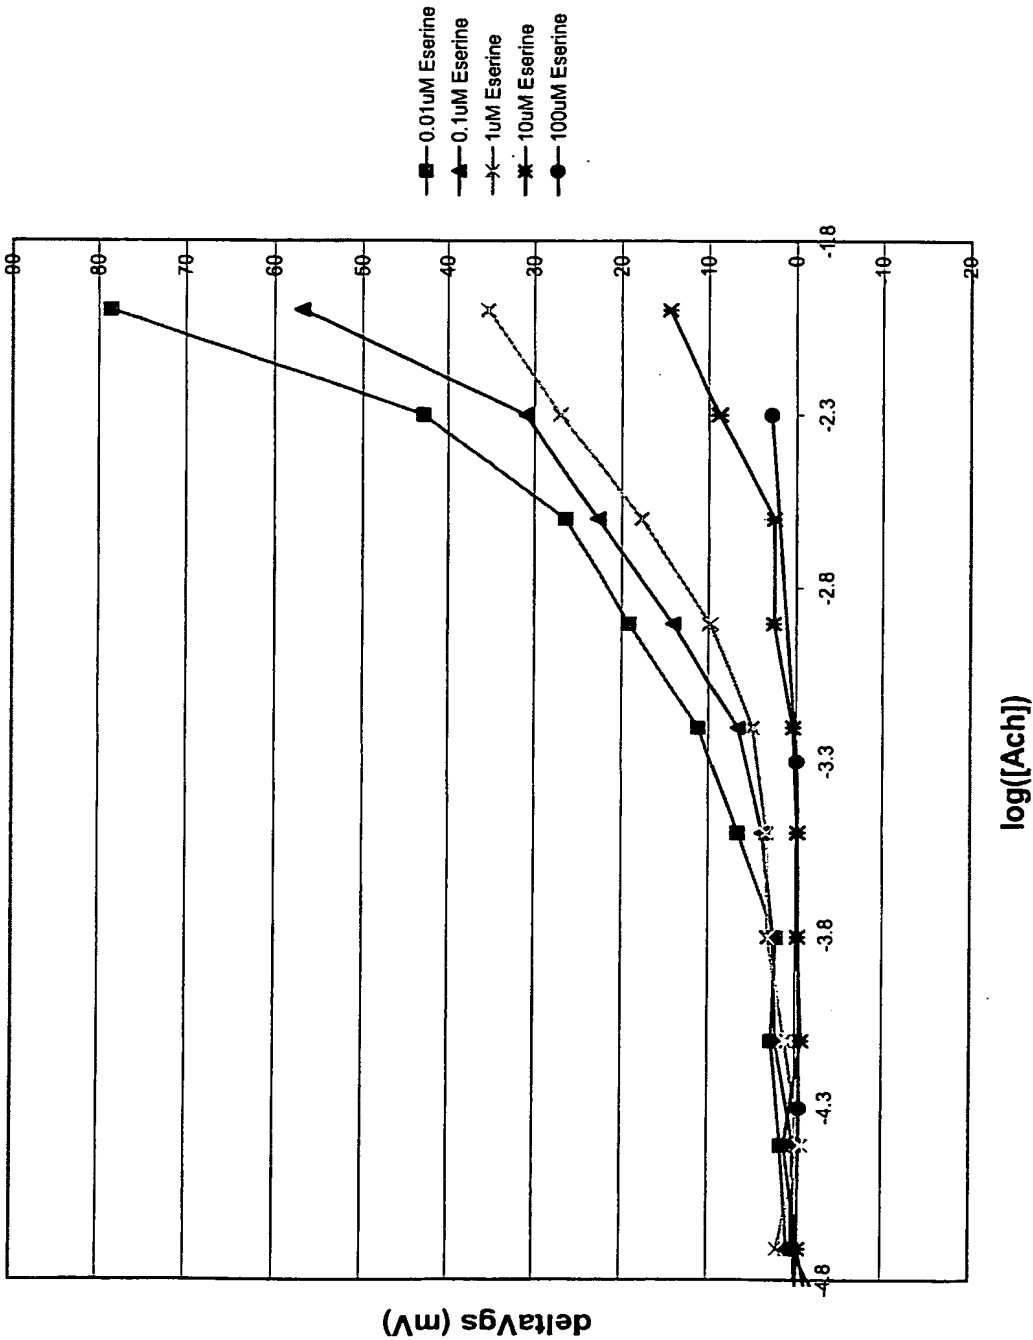


FIG. 6

6/14

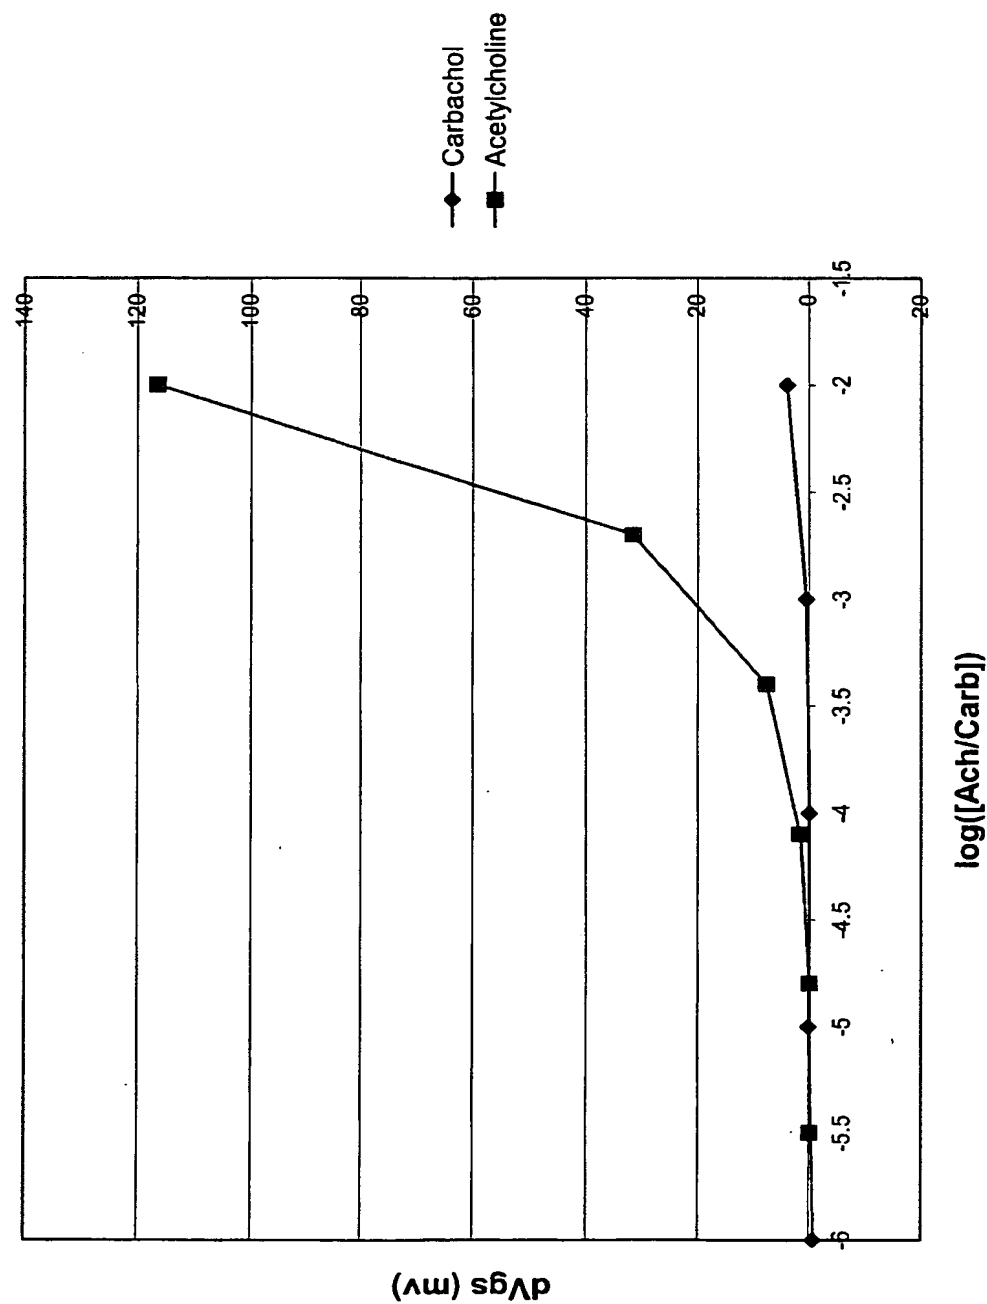


FIG. 7

7/14

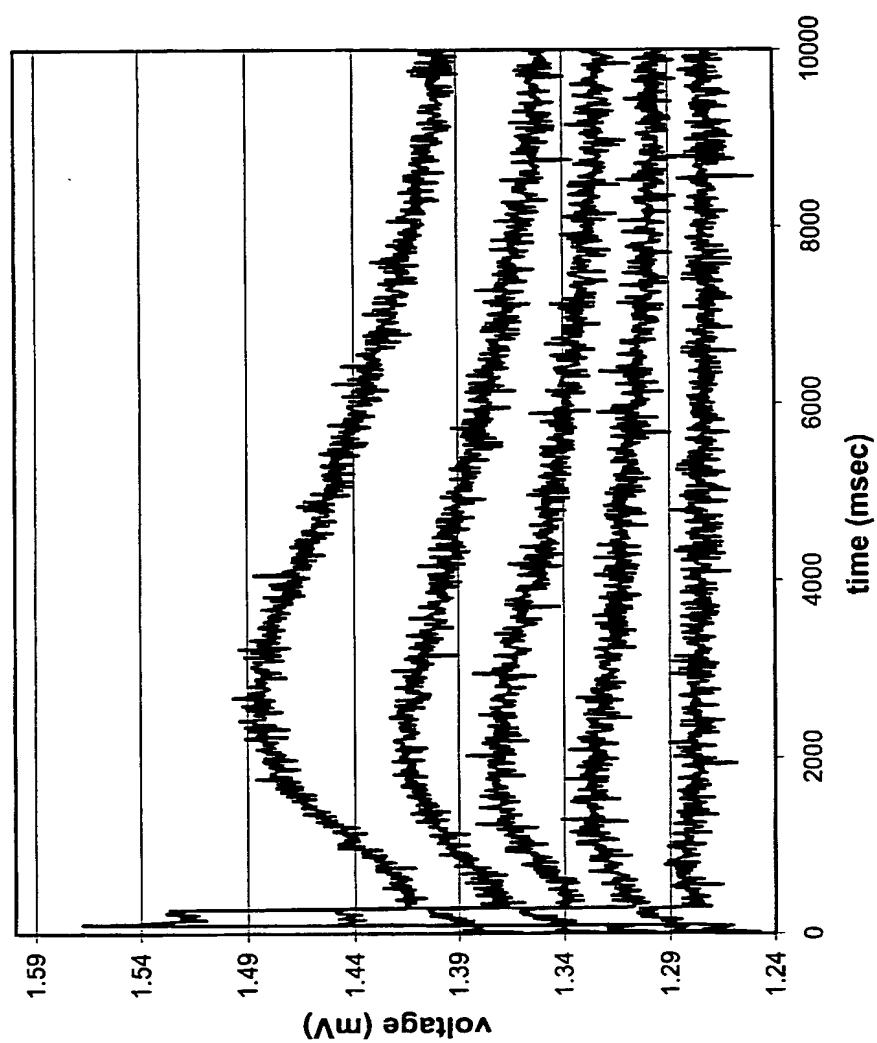


FIG. 8

8/14

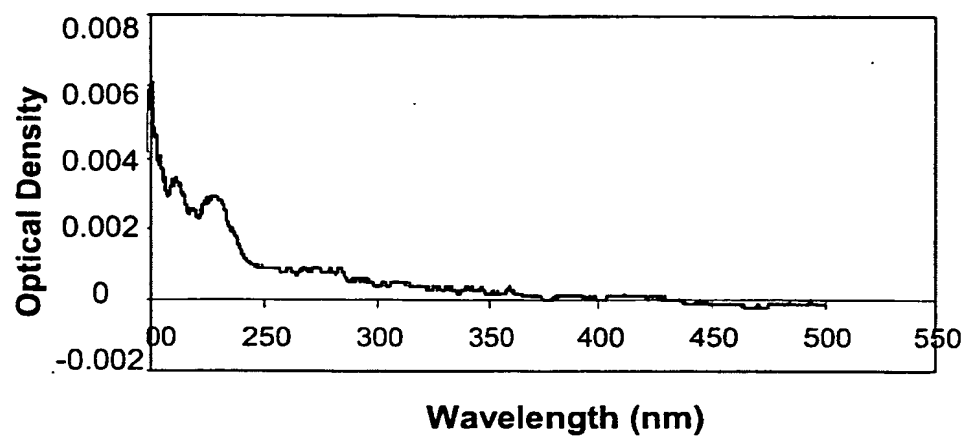


FIG. 9

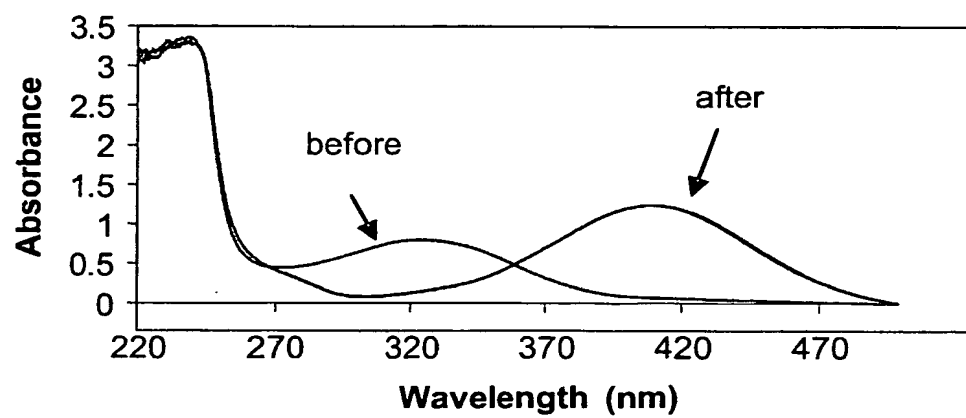


FIG. 10

9/14

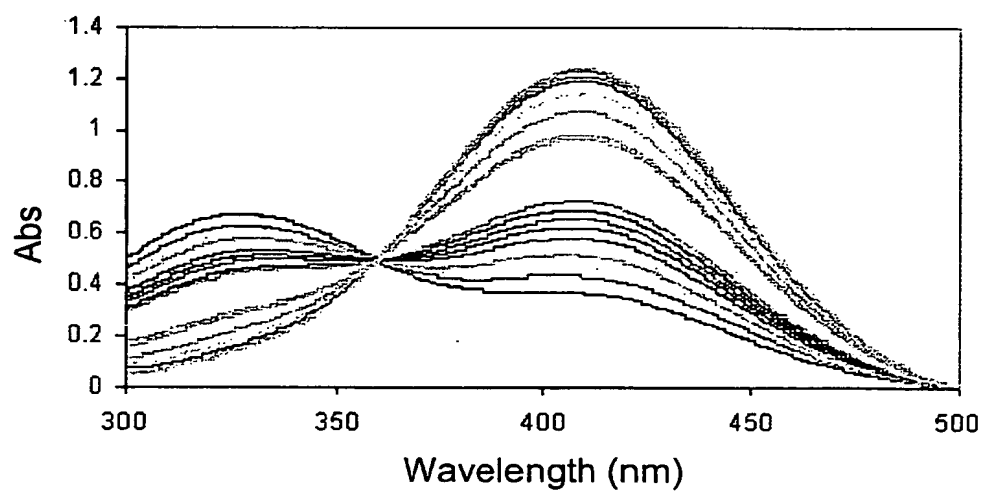


FIG. 11

10/14

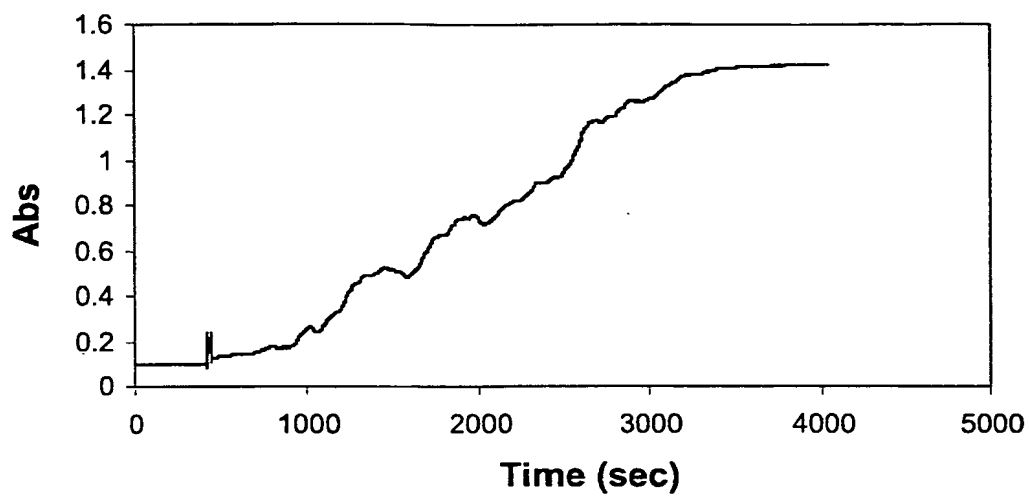


FIG. 12

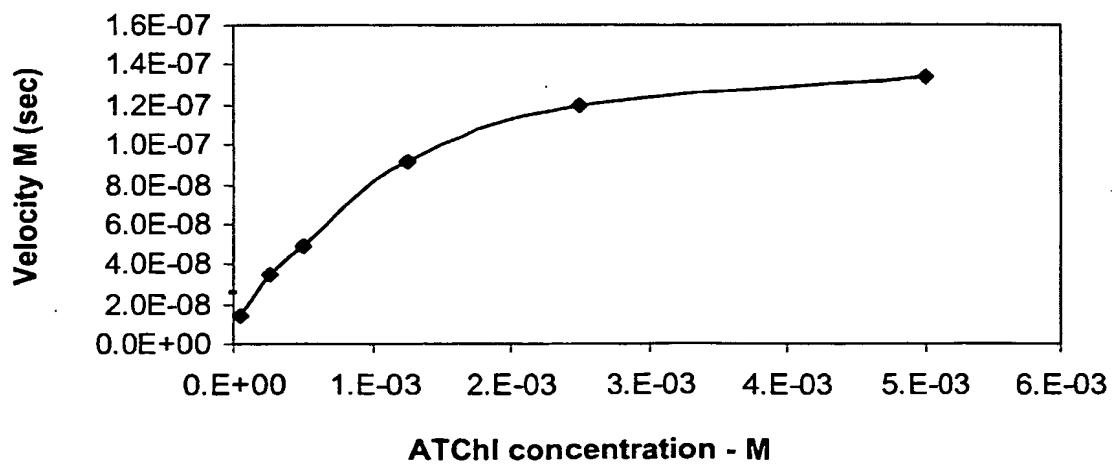


FIG. 13

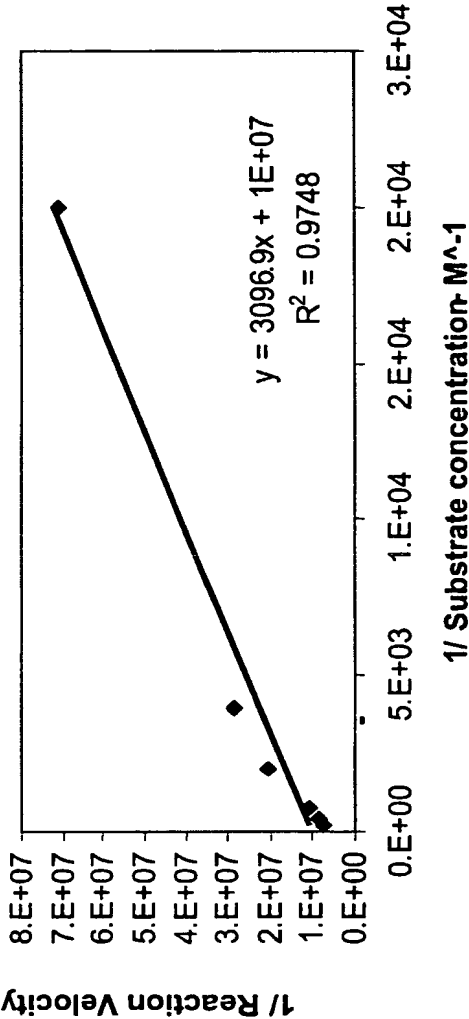


FIG.14

12/14

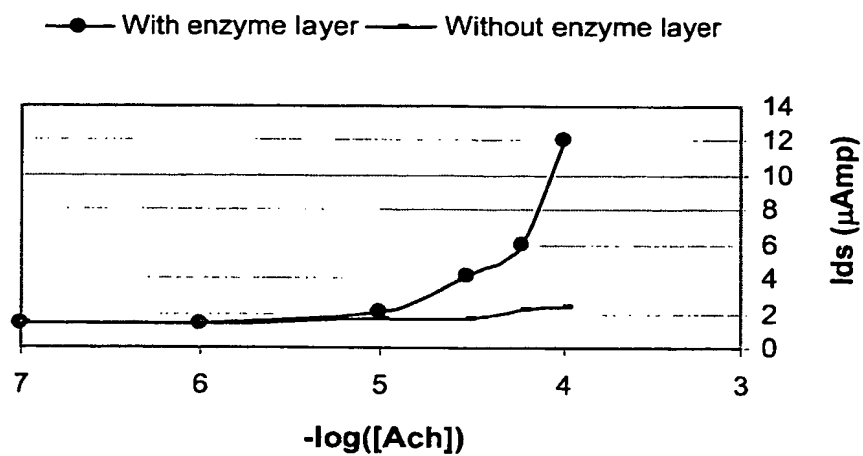


FIG. 15A

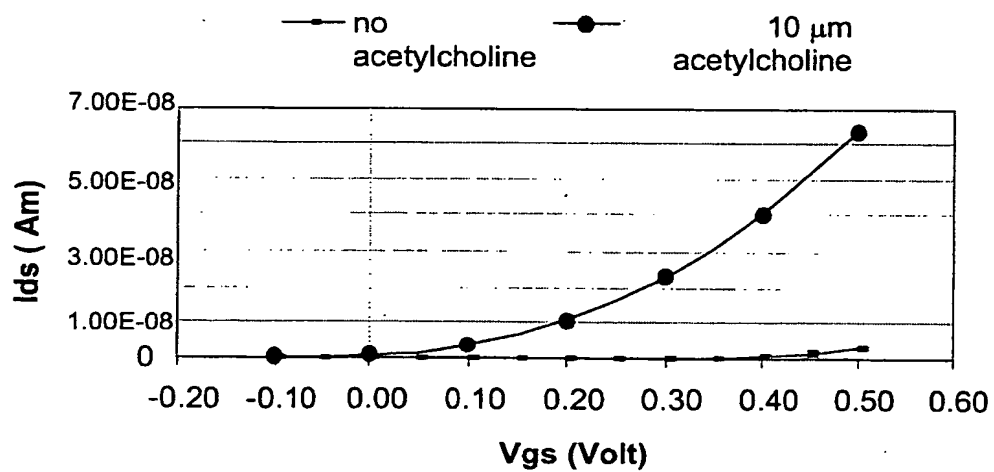


FIG. 15B

13/14

FIG. 16A

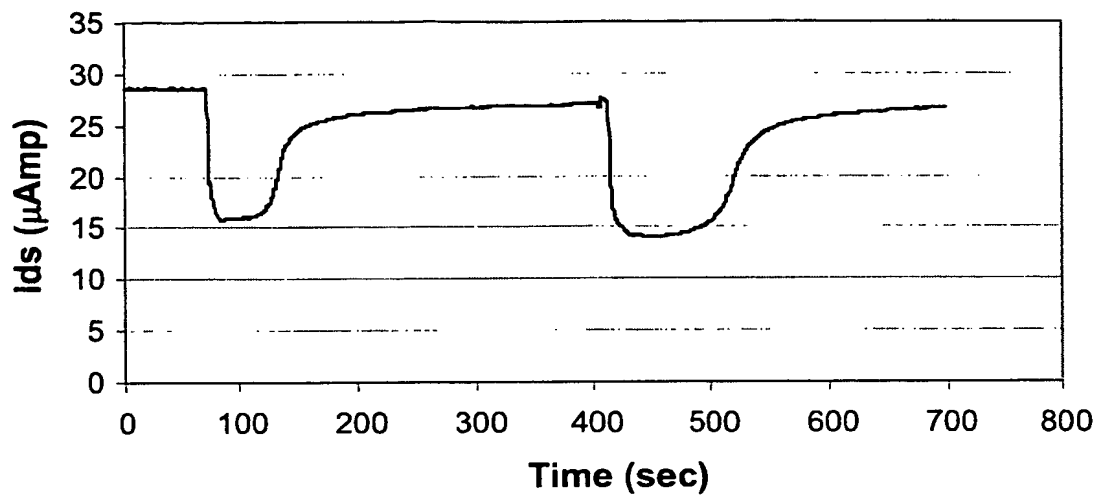
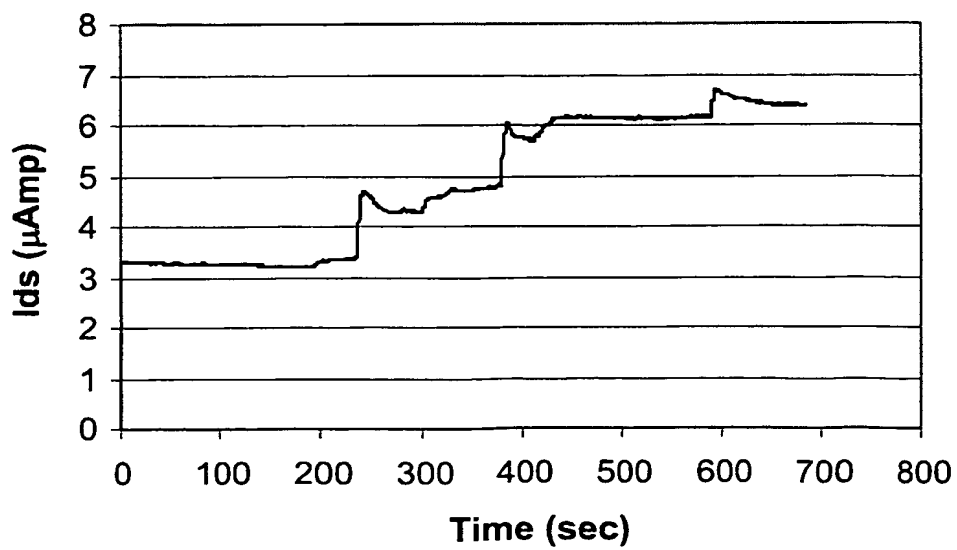


FIG. 16B



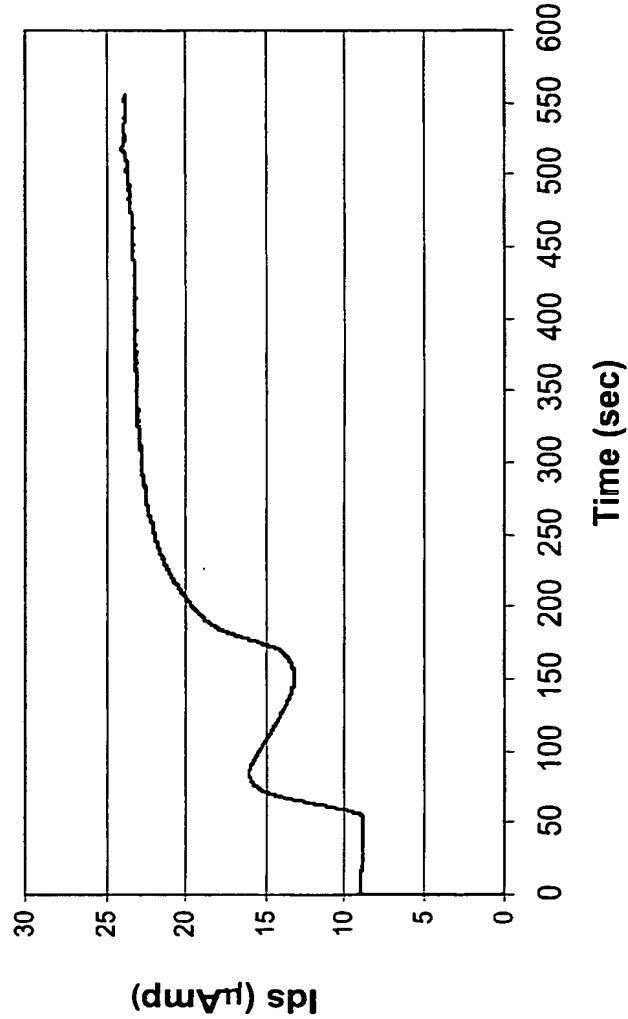


FIG.17

INTERNATIONAL SEARCH REPORT

Int'l Application No

PCT/IL 03/00941

A. CLASSIFICATION OF SUBJECT MATTER
 IPC 7 G01N27/414 G01N33/543

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G01N C07K C12Q

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ, CHEM ABS Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	KHARITONOV ANDREI B ET AL: "Enzyme monolayer-functionalized field-effect transistors for biosensor applications" SENS ACTUATORS, B CHEM; SENSORS AND ACTUATORS, B: CHEMICAL NOV 2000 ELSEVIER SEQUOIA SA, LAUSANNE, SWITZERLAND, vol. 70, no. 1-3, November 2000 (2000-11), pages 222-231, XP0004224603	1-11, 15, 16
Y	abstract; schemes 2,3; paragraph joining pages 227 and 228; figure 4 ----- -/-	1-16

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

15 March 2004

Date of mailing of the international search report

30/03/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
 NL - 2280 HV Rijswijk
 Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
 Fax: (+31-70) 340-3016

Authorized officer

Fausti, S

INTERNATIONAL SEARCH REPORT

Int. Application No.

PCT/IL 03/00941

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	TORBICZ W ET AL: "pH-ISFET based urea biosensor" SENSORS AND ACTUATORS B, ELSEVIER SEQUOIA S.A., LAUSANNE, CH, vol. 44, no. 1-3, 1 October 1997 (1997-10-01), pages 370-376, XP004117167 ISSN: 0925-4005	1-4, 8-11,15, 16
Y	abstract; page 370, left-hand column, lines 5-7; paragraphs joining pages 370-371 and 371-372; figure 7; table 1	1-4,8-16
Y	US 4 562 157 A (EARLEY FERGUS G P ET AL) 31 December 1985 (1985-12-31) abstract; column 2, lines 58-65; column 4, lines 2-7; reaction schemes joining columns 4-5 and 8-9; column 9, lines 7-14	12-14
A	HASEBE, Y. ET AL: "Tyrosinase -immobilized carbon felt as a flow through bioelectrochemical detector for phenol, catechol and its inhibiting species" CHEMICAL SENSORS , 17(SUPPL. B), 117-119 CODEN: KAGSEU, 2001, XP0009027649 abstract	11
Y	SAKAI HIROMITSU ET AL: "Analytical application for chemicals using an enzyme sensor based on an ISFET" SENS ACTUATORS, B CHEM; SENSORS AND ACTUATORS, B: CHEMICAL JUN 1993, vol. B14, no. 1-3 part 2, 13 September 1992 (1992-09-13), pages 578-580, XP0009027631 page 578, paragraph joining left- and right-hand columns; figures 1,3,5	1-16
A	WO 88/09499 A (UNIV JOHNS HOPKINS) 1 December 1988 (1988-12-01) figure 4	

INTERNATIONAL SEARCH REPORT

Information on patent family members

Int'l Patent Application No.

PCT/IL 03/00941

Patent document cited in search report		Publication date		Patent family member(s)	Publication date
US 4562157	A	31-12-1985	CA	1229883 A1	01-12-1987
			DE	3468146 D1	28-01-1988
			DK	256784 A	26-11-1984
			EP	0127438 A1	05-12-1984
			GB	2141544 A ,B	19-12-1984
			JP	1933206 C	26-05-1995
			JP	6050316 B	29-06-1994
			JP	59225343 A	18-12-1984
<hr/>					
WO 8809499	A	01-12-1988	US	4822566 A	18-04-1989
			EP	0363401 A1	18-04-1990
			JP	2504069 T	22-11-1990
			WO	8809499 A1	01-12-1988
<hr/>					

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

☐ **BLACK BORDERS**

☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**

☒ **FADED TEXT OR DRAWING**

☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**

☒ **SKEWED/SLANTED IMAGES**

☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**

☐ **GRAY SCALE DOCUMENTS**

☒ **LINES OR MARKS ON ORIGINAL DOCUMENT**

☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**

☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.